


OSL-2.92-M-43.5G

2.92mm Plug 50ohm Open Short Load 43.5GHz

50Ω

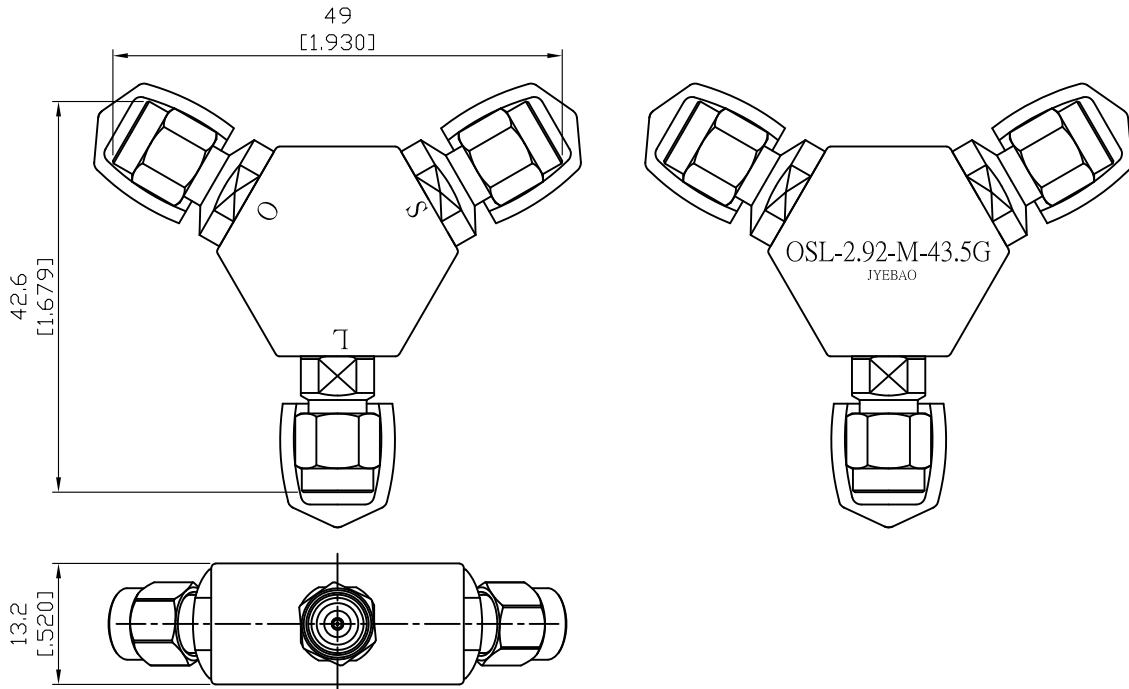

OPEN				
FREQUENCY RANGE	DC-43.5GHz			
IMPEDANCE	50Ω			
OFFSET LENGTH	Agilent 16.70ps	Anritsu 5.01mm	Rohde & Schwarz 5.01mm	
CAPACITANCE	Agilent / Anritsu		Rohde & Schwarz	
C0	(1E-15) F	4.500	fF	4.5000000
C1	(1E-27) F/Hz	395.000	fF/GHz	0.3950000
C2	(1E-36) F/Hz <sup>2</sup>	-20.000	fF/GHz <sup>2</sup>	-0.0200000
C3	(1E-45) F/Hz <sup>3</sup>	0.400	fF/GHz <sup>3</sup>	0.0004000
PHASE ERROR	DC-6GHz	≤ 1°		
	6-26.5GHz	≤ 3°		
	26.5-40GHz	≤ 5°		
	40-43.5GHz	≤ 6°		
RETURN LOSS	DC-18GHz	≤ 0.10dB		
	18-43.5GHz	≤ 0.25dB		

SHORT				
FREQUENCY RANGE	DC-43.5GHz			
IMPEDANCE	50Ω			
OFFSET LENGTH	Agilent 16.70ps	Anritsu 5.01mm	Rohde & Schwarz 5.01mm	
INDUCTANCE	Agilent / Anritsu		Rohde & Schwarz	
L0	(1E-12) H	4.000	pH	4.0000000
L1	(1E-24) H/Hz	-650.000	pH/GHz	-0.6500000
L2	(1E-33) H/Hz <sup>2</sup>	39.000	pH/GHz <sup>2</sup>	0.0390000
L3	(1E-42) H/Hz <sup>3</sup>	-0.640	pH/GHz <sup>3</sup>	-0.0006400
PHASE ERROR	DC-6GHz	≤ 1°		
	6-26.5GHz	≤ 3°		
	26.5-40GHz	≤ 5°		
	40-43.5GHz	≤ 6°		
RETURN LOSS	DC-18GHz	≤ 0.10dB		
	18-43.5GHz	≤ 0.25dB		

LOAD		
FREQUENCY RANGE	DC-43.5GHz	
IMPEDANCE	50Ω	
DC RESISTANCE	50±0.25Ω	
MAX POWER	0.25W	
RETURN LOSS	DC-6GHz	≥ 42dB
	6-43.5GHz	≥ 30dB

**Notes:**

1. Temperature range for optimal results: +20 °C to +26 °C
2. Storage temperature range: -20 °C to +75 °C
3. When not in use put on cap to keep connector clean
4. Return loss test results shipped along with goods (example below)

Parts	Material	Plating ( Micro-inch )
Housing	Aluminium	Anodized (Green)
Cap	PVC	
Body open/short/load	Stainless Steel	Passivated
Contact pin open/short/load	Beryllium Copper	Gold 4 Over Nickel Phosphorous Alloy 80 Over Copper 20
Dielectric load/open	PPO	

This part number complies with RoHS.

Notice: JYEBAO reserves the right to make modifications deemed appropriate.


Test equipment

N5227B NETWORK ANALYZER


Return Loss

OSL-2.92-M-43.5G test result


Open

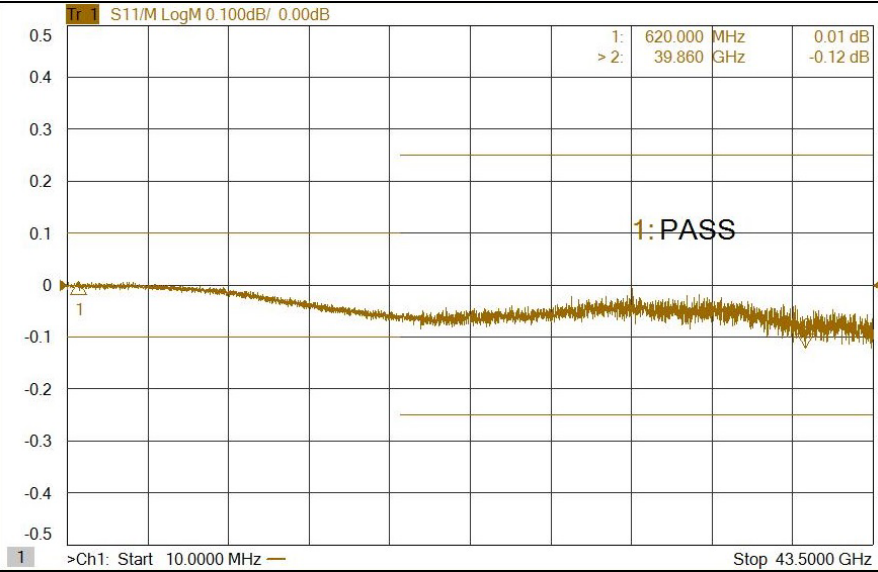

Short

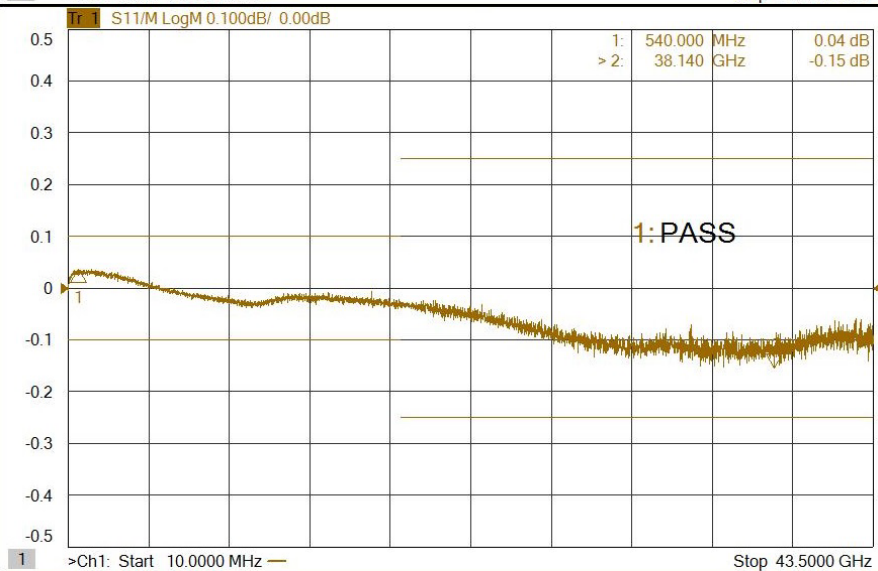

Load

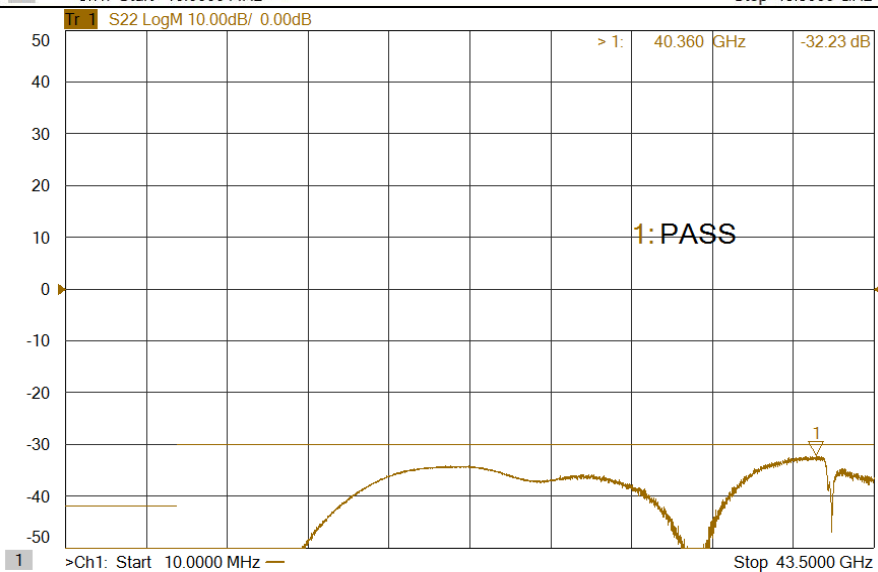


Test equipment

N5227B NETWORK ANALYZER

Phase error

TOSLK50A-43.5 VS OSL-2.92-M-43.5G

Open

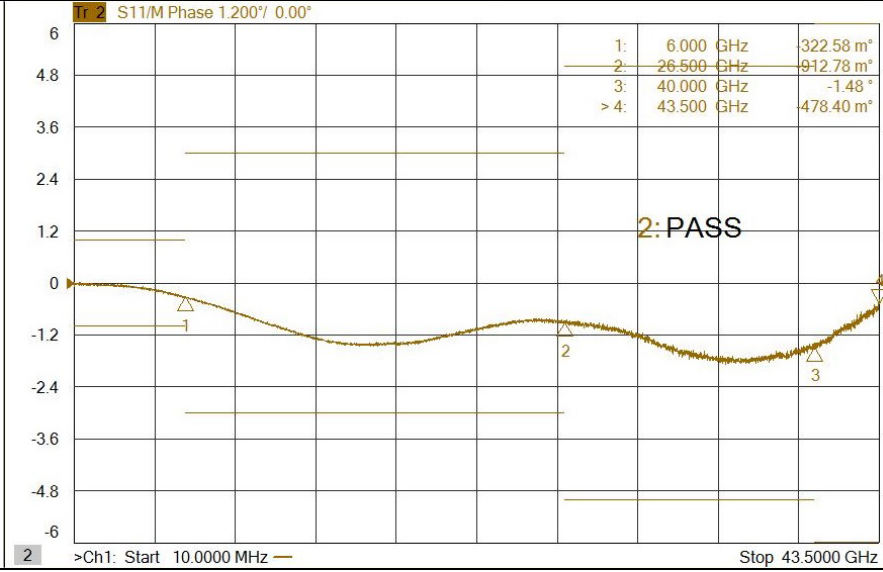

Short

